




SUPPORTED SCAN BODIES – BIOHORIZONS INTERNAL HEX

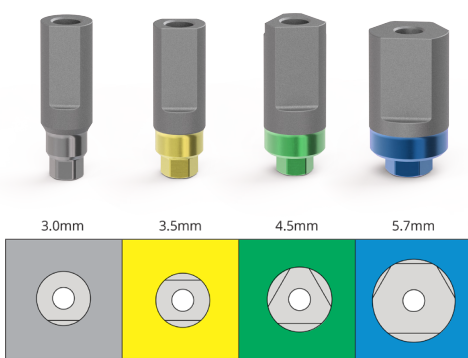

BioHorizons Titanium Scan Bodies
TP3TSB, PYTSB, PGTSB, PBTSB

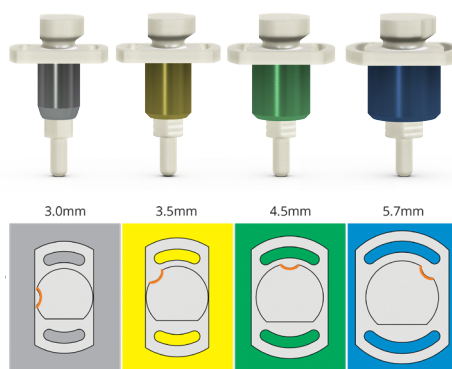


BioHorizons 8mm Snap Scan Bodies
TP3SSB8, PYSSB8, PGSSB8, PBSSB8

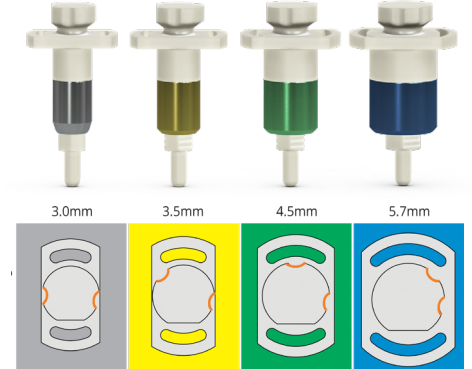


BioHorizons 11mm Snap Scan Bodies
TP3SSB11, PYSSB11, PGSSB11, PBSSB11



BioHorizons Snap Scan Bodies
TP3SSB, PYSSB, PGSSB, PBSSB

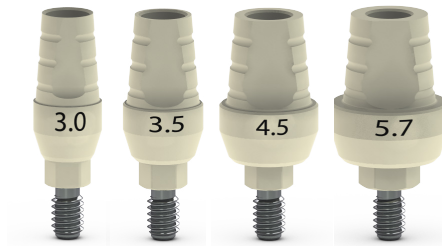

BioHorizons PEEK Scan Bodies
TP3PSA, PYPSA, PGPSA, PBPSA

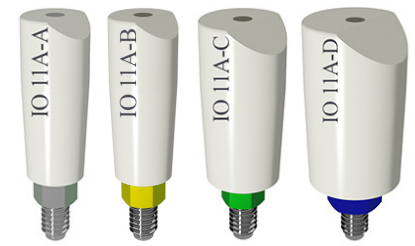

Elos IO Scan Bodies
IO-11A-A, IO-11A-B, IO-11A-C, IO-11A-D



DESS Intraoral Scan Bodies
52.099, 52.087, 52.088, 52.089



3Shape Scan Bodies
BI3, BIY, BIG, BIB



NT Trading 3D-Guide Scan Body
*BIO 9.S3D3.000, BIO 9.S3D3.500,
 BIO 9.S3D4.500, BIO 9.S3D5.700*



Anatotemp SC – Internal Hex
*1035-01SC, 1035-02SC, 1035-03SC, 1035-04SC,
 1045-01SC, 1045-03SC, 1045-04SC, 1045-05SC,
 1045-06SC, 1057-05SC, 1057-06SC*

SUPPORTED SCAN BODIES – BIOHORIZONS MULTI-UNIT



BioHorizons Titanium Scan Body
PXMUTSB



Elos IO Scan Body
IO-11B-A



Open Implants Scan Body
3915



BioHorizons Contoured Cover Cap
PXMUCCC
**not recommended for
full arch intra-oral scanning*



BioHorizons Cover Cap
PXMUCC
**not recommended for
full arch intra-oral scanning*



Imetric MU
**Bar library only*

**Open Implants image sourced from Open Implants.
*3Shape scan body image sourced from 3Shape.
*DESS Intraoral Scan Body image sourced from DESS.
*NT Trading 3D-Guide Scan Body sourced from NT Trading.
Imetric MU rendering created by Vulcan Custom Dental.